


14 LJ2004100007

Catalog No : CS-0033199 Batch# Ld0410021A-RP-519 JLW

Sample Name:	LJ2004100007	Injection Volume:	2.0
Vial Number:	RE4	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90A 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2020-4-10 18:56	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

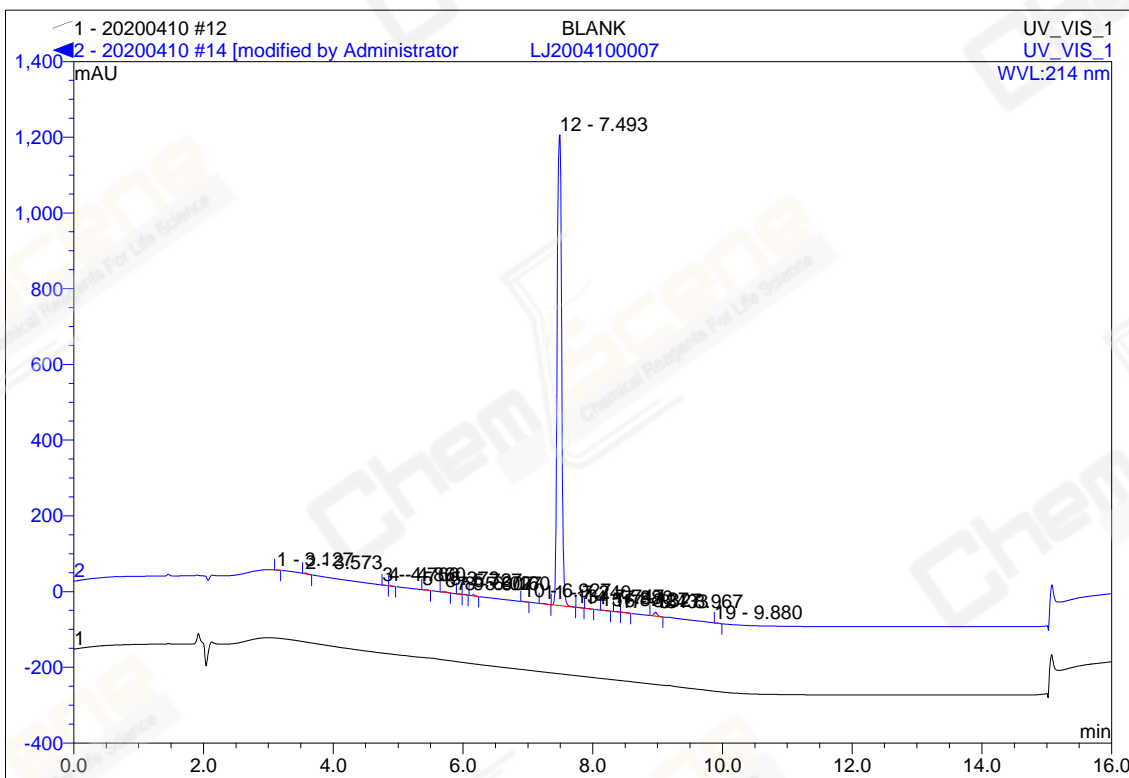

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	3.13	n.a.	0.411	0.022	0.02	n.a.	BMB*
2	3.57	n.a.	1.886	0.086	0.09	n.a.	BMB*
3	4.76	n.a.	0.006	0.017	0.02	n.a.	BMB*
4	4.86	n.a.	0.022	0.020	0.02	n.a.	BMB*
5	5.37	n.a.	0.007	0.054	0.05	n.a.	BMB
6	5.73	n.a.	1.826	0.107	0.11	n.a.	BMB
7	5.91	n.a.	0.031	0.015	0.01	n.a.	BMB*
8	6.03	n.a.	1.161	0.052	0.05	n.a.	bMB*
9	6.16	n.a.	3.054	0.138	0.14	n.a.	BMB
10	6.93	n.a.	0.637	0.046	0.05	n.a.	BMB*
11	7.24	n.a.	1.398	0.085	0.09	n.a.	BMB
12	7.49	n.a.	1244.022	97.863	98.49	n.a.	BMB
13	7.75	n.a.	0.033	0.048	0.05	n.a.	BMB*
14	7.88	n.a.	0.005	0.028	0.03	n.a.	BMB*
15	8.13	n.a.	0.021	0.036	0.04	n.a.	BMB*

16	8.33	n.a.	0.008	0.021	0.02	n.a.	BMB*
17	8.43	n.a.	0.006	0.046	0.05	n.a.	bMB*
18	8.97	n.a.	10.449	0.634	0.64	n.a.	BMB
19	9.88	n.a.	0.035	0.041	0.04	n.a.	BMB*
Total:			1265.016	99.359	100.00	0.000	