
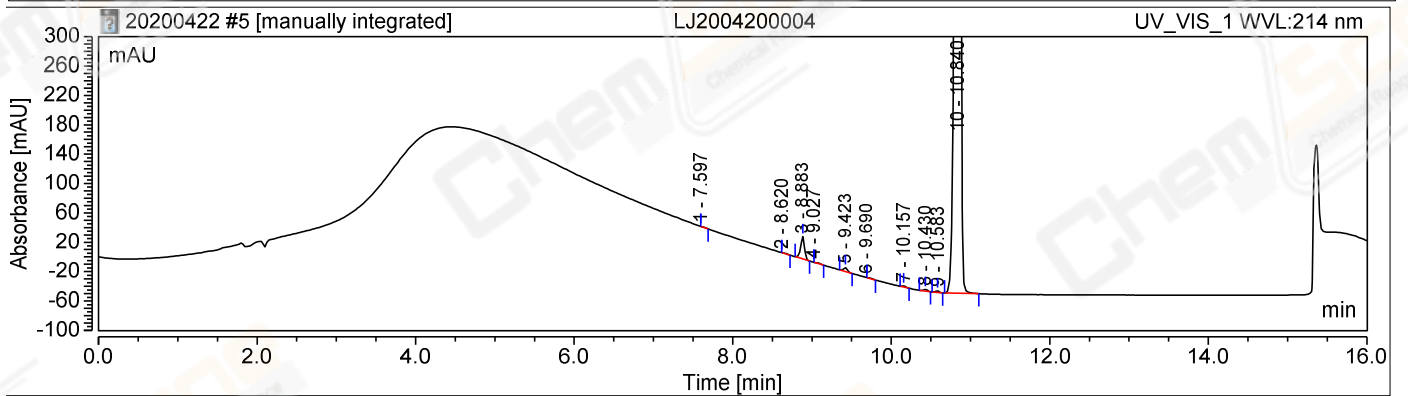


## Chromatogram and Results

Injection Details		
Injection Name:	LJ2004200004	Run Time (min): 16.00
Vial Number:	GA6	Users: ly
Injection Type:	Unknown	Injection Volume: 2.00
Calibration Level:		Channel: UV_VIS_1
Instrument Method:	10-90A,214NM	Wavelength: 214
Processing Method:	3D Quantitative	Bandwidth: 4
CAS NO.:	488-23-3	Dilution Factor: 1.0000
Injection Date/Time:	22/Apr/20 14:37	Sample Weight: 1.0000
chrom://hy442/ATA2/Instrument Data/202004/20200422.seq/538.smp/UV_VIS_1.channel/UV_VIS_1.chm		

### Chromatogram

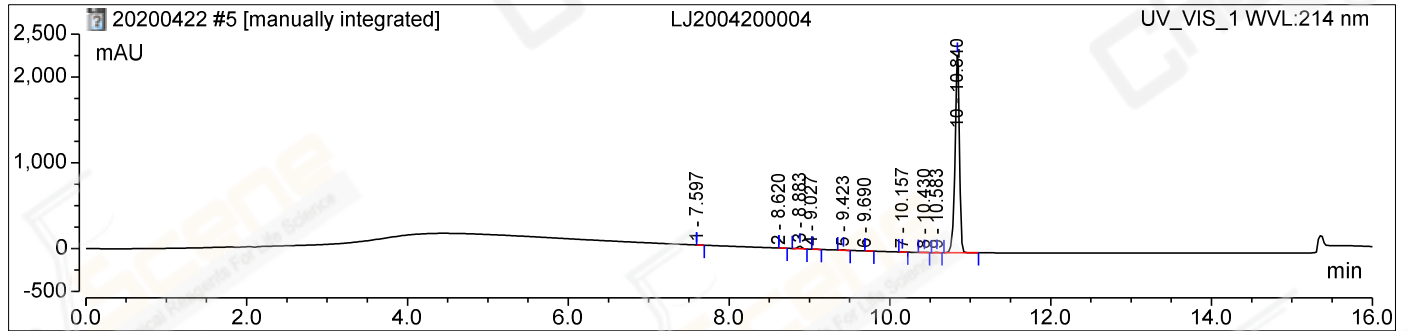

### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Match	Resolution (EP)	Asymmetry (EP)	Rel.Area %
1		7.597	0.024	0.000	1000	n.a.	n.a.	0.02
2		8.620	0.031	0.000	0	n.a.	n.a.	0.02
3		8.883	1.725	30.212	1000	n.a.	0.90	1.15
4		9.027	0.066	0.000	1000	n.a.	n.a.	0.04
5		9.423	0.301	5.281	997	n.a.	0.97	0.20
6		9.690	0.040	0.000	0	n.a.	n.a.	0.03
7		10.157	0.079	1.570	957	3.24	1.14	0.05
8		10.430	0.136	2.423	989	1.78	0.96	0.09
9		10.583	0.130	2.477	979	2.81	0.94	0.09
10		10.840	148.072	2304.480	968	n.a.	0.88	98.32
Total:			150.605	2346.443			7.83	5.77