


51 CPK2019-221-14169			
Catalog No: CS-M2997 Batch#14169		A-RP-301 GWW	
Sample Name:	CPK2019-221-14169	Injection Volume:	5.0
Vial Number:	GD8	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	220
Control Program:	30-90A 220NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-2-21 23:39	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

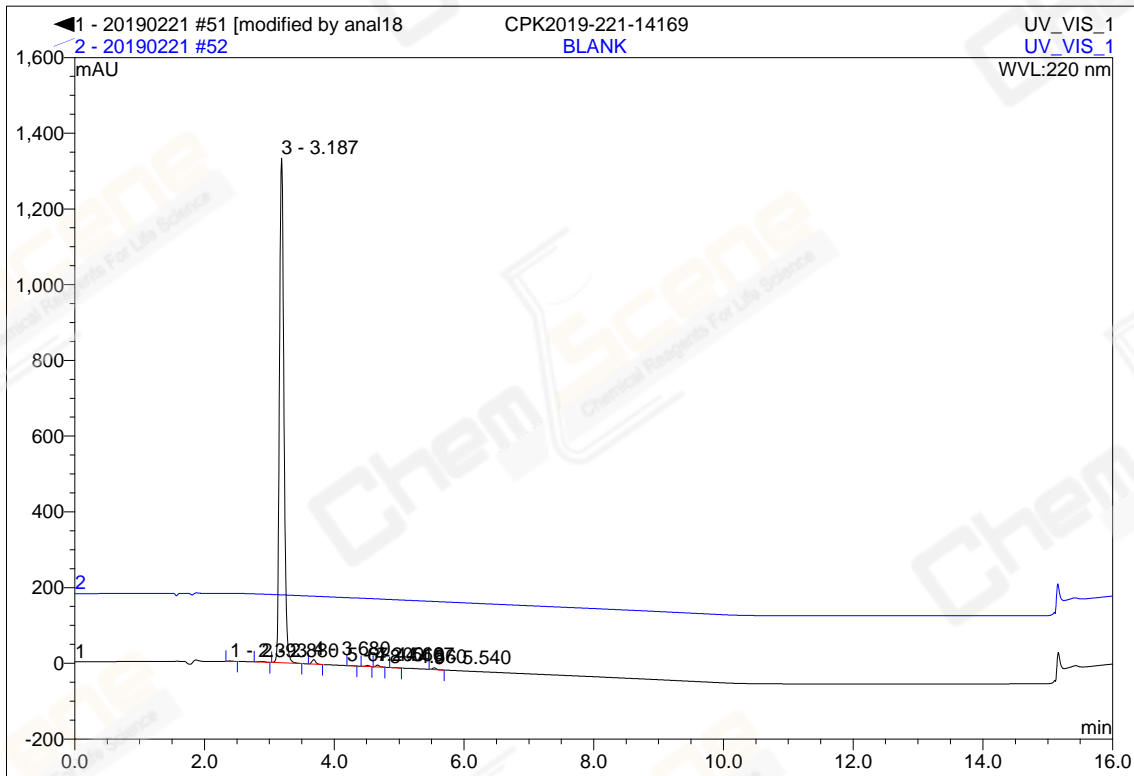

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	2.39	n.a.	1.025	0.080	0.07	n.a.	BMB*
2	2.88	n.a.	1.919	0.162	0.15	n.a.	BMB*
3	3.19	n.a.	1333.409	105.736	98.25	n.a.	BMB*
4	3.68	n.a.	11.992	0.823	0.76	n.a.	BMB*
5	4.20	n.a.	0.021	0.031	0.03	n.a.	BMB*
6	4.51	n.a.	2.690	0.166	0.15	n.a.	BMB*
7	4.67	n.a.	4.695	0.303	0.28	n.a.	BMB*
8	4.86	n.a.	0.002	0.034	0.03	n.a.	BMB
9	5.54	n.a.	4.626	0.290	0.27	n.a.	BMB
Total:			1360.379	107.625	100.00	0.000	