
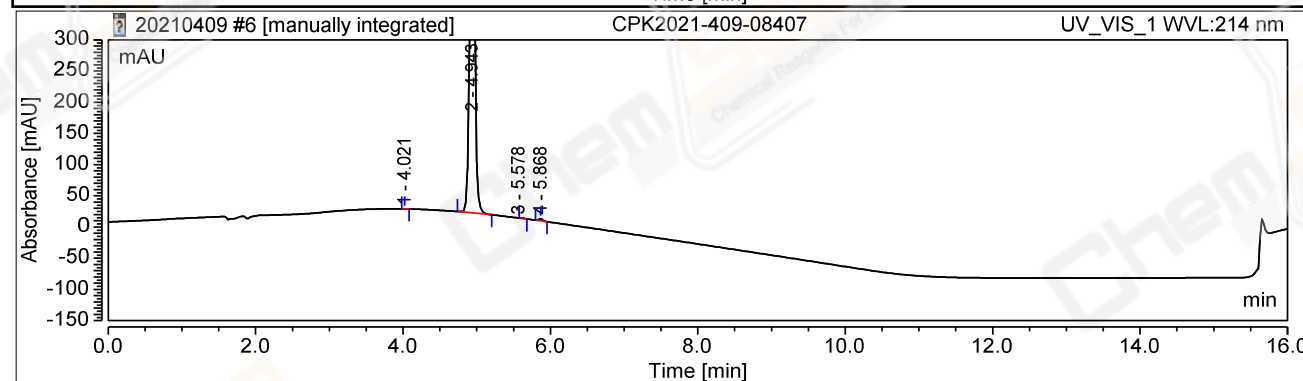


Chromatogram and Results

Injection Details	
Injection Name: CPK2021-409-08407	Injection Volume: 2.00
Vial Number: BD2	Channel: UV_VIS_1
Injection Type: Unknown	Wavelength: 214
Calibration Level:	Users: zhouxin
Instrument Method: 30-90A,214NM	Dilution Factor: 1.0000
Processing Method: New Processing Method	Sample Weight: 1.0000
Injection Date/Time: 09/Apr/21 15:06	Run Time (min): 16.00
CAS NO.: 865663-98-5 A-RP-541	
chrom://hy261/Themo/Instrument Data/202104/20210409.seq/696.smp/UV_VIS_1.channel/UV_VIS_1.chm	

Chromatogram

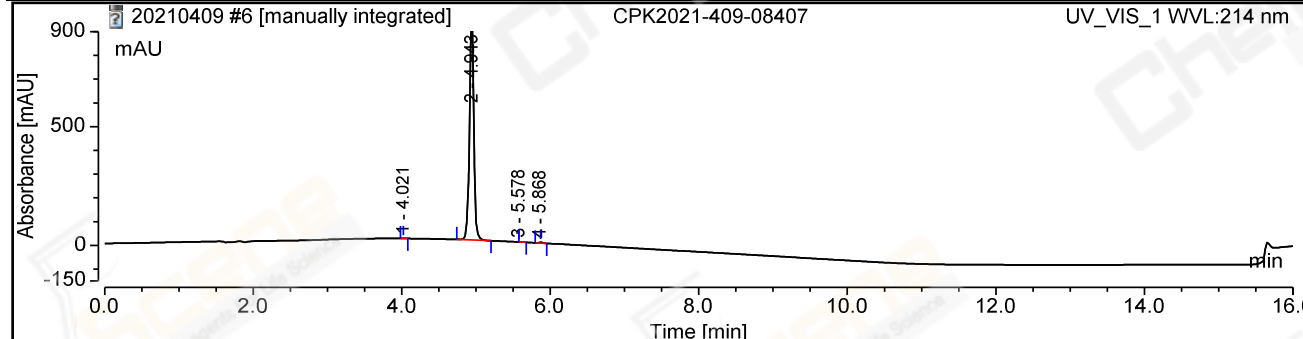

Integration Results							
No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Plates (EP)	Rel.Area %
1		4.021	0.012	0.250	1.18	47393	0.02
2		4.943	62.861	948.293	0.96	39572	99.63
3		5.578	0.028	0.000	n.a.	n.a.	0.04
4		5.868	0.191	3.471	0.99	75732	0.30
Total:			63.092	952.015	3.13		