


<b>2 CPK2018-620-18404</b>			
<b>CAS NO.: 1234015-52-1 A-RP-301</b>			
Sample Name:	CPK2018-620-18404	Injection Volume:	5.0
Vial Number:	BA2	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	290
Control Program:	HM-414_13-H01P01(RP-HPLC)	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2018-6-21 13:33	Sample Weight:	1.0000
Run Time (min):	21.00	Sample Amount:	1.0000

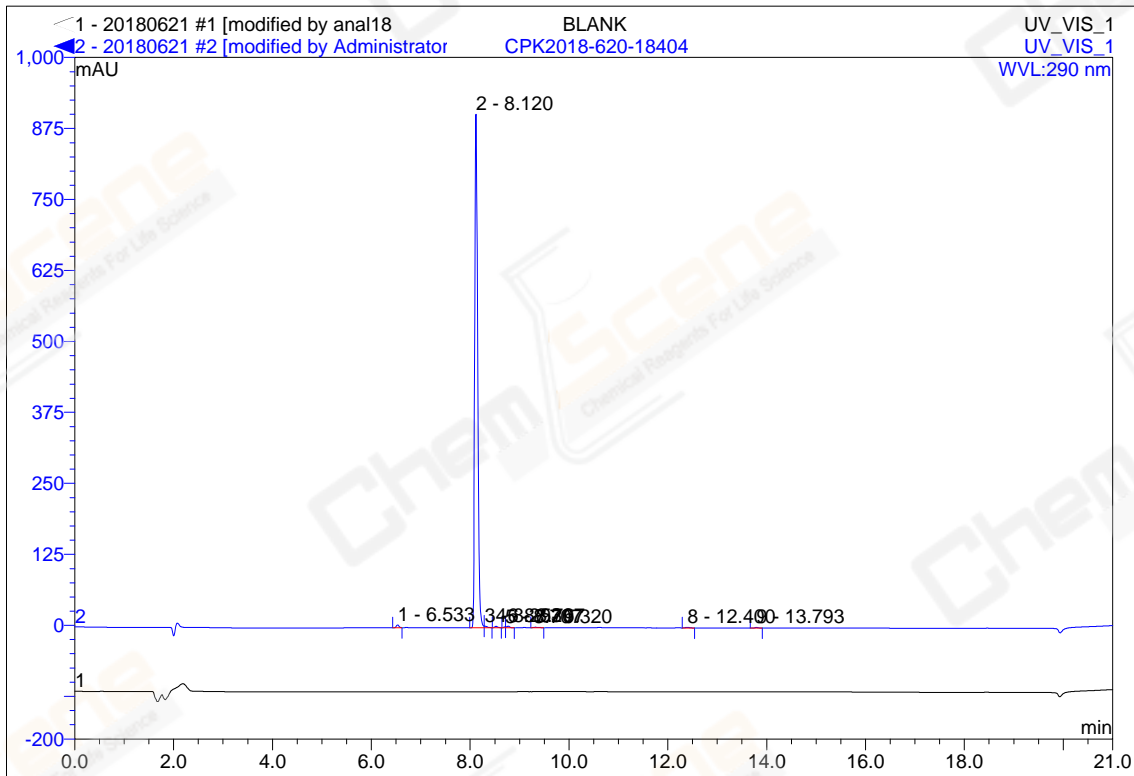

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	6.53	n.a.	4.723	0.285	0.45	n.a.	BMB*
2	8.12	n.a.	904.287	62.130	98.22	n.a.	BM *
3	8.29	n.a.	2.715	0.169	0.27	n.a.	MB*
4	8.52	n.a.	2.279	0.151	0.24	n.a.	BMB*
5	8.71	n.a.	1.417	0.050	0.08	n.a.	BM *
6	8.77	n.a.	2.634	0.202	0.32	n.a.	MB*
7	9.32	n.a.	0.760	0.093	0.15	n.a.	BMB*
8	12.40	n.a.	0.989	0.102	0.16	n.a.	MB*
9	13.79	n.a.	0.912	0.073	0.12	n.a.	BMB*
<b>Total:</b>			920.716	63.255	100.00	0.000	