
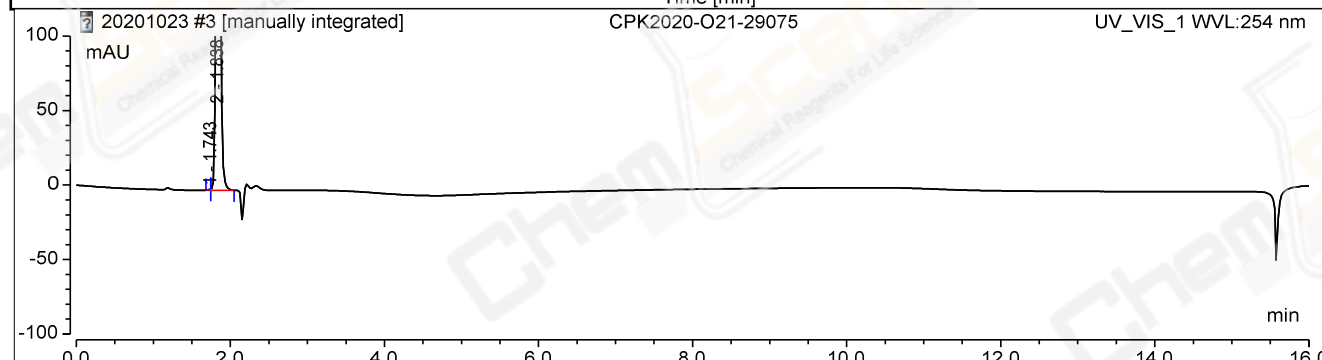


Chromatogram and Results

Injection Details			
Injection Name:	CPK2020-O21-29075	Injection Volume:	2.00
Vial Number:	RB2	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	254
Calibration Level:		Users:	ghj
Instrument Method:	10-90A,254NM	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	23/Oct/20 10:56	Run Time (min):	16.00
Comment:	HY-081_34-20180306 A-RP-541		
chrom://hy261/Themo/Instrument Data/202010/20201023.seq/722.smp/UV_VIS_1.channel/UV_VIS_1.chm			

Chromatogram

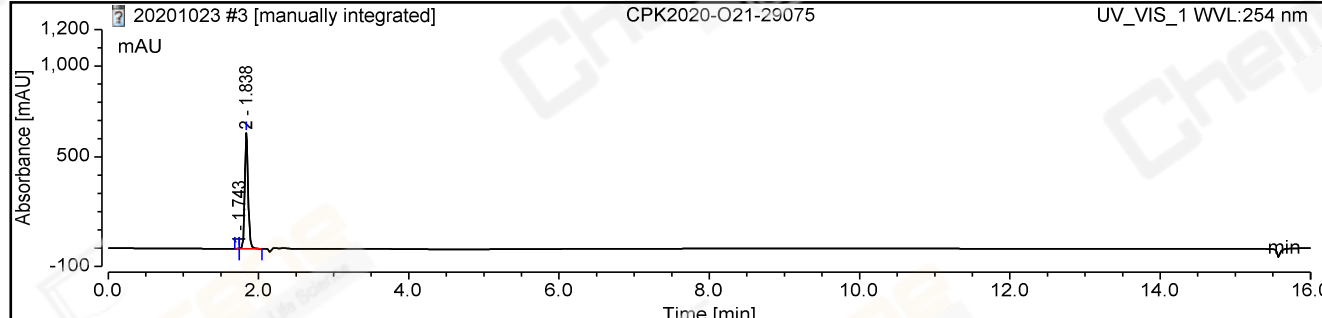

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	S/N	Rel.Area %
1		1.743	0.022	0.607	n.a.	3.6	0.07
2		1.838	31.866	634.827	1.16	3750.0	99.93
Total:			31.888	635.433	1.16	3753.59	