
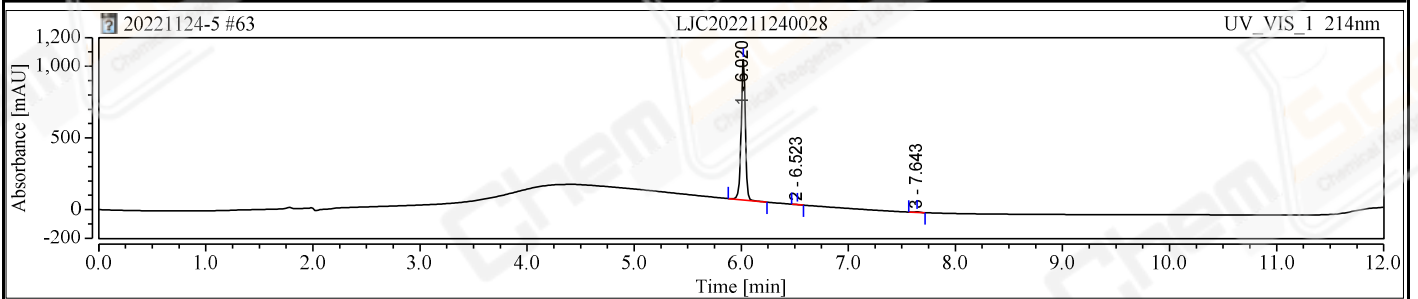


Chromatogram and Results

Sample ID: LJC202211240028	CAS NO.: 14544-47-9
Batch No:	Channel: UV_VIS_1
Vial Number: BA7	Wavelength: 214.0
Injection Type: Unknown	Injection Volume: 5.00
Instrument: LC10410	Injection Time: 25/11/2022 01:23
Instrument Method: 10-80A-12min(LP-HPLC)	InstMeth.creation_t 15/04/2022 17:33
Processing Method: LJC202211240028	Last update_time: 25/11/2022 11:13
seq.creation_operator: Mshaor	
chrom://ahqc015/CMDATA/Instrument Data/LC10410/Leyan/Sequence/202211/20221124-5.seq/559.smp/UV_VIS_1.channel/UV_VIS_1.chm	

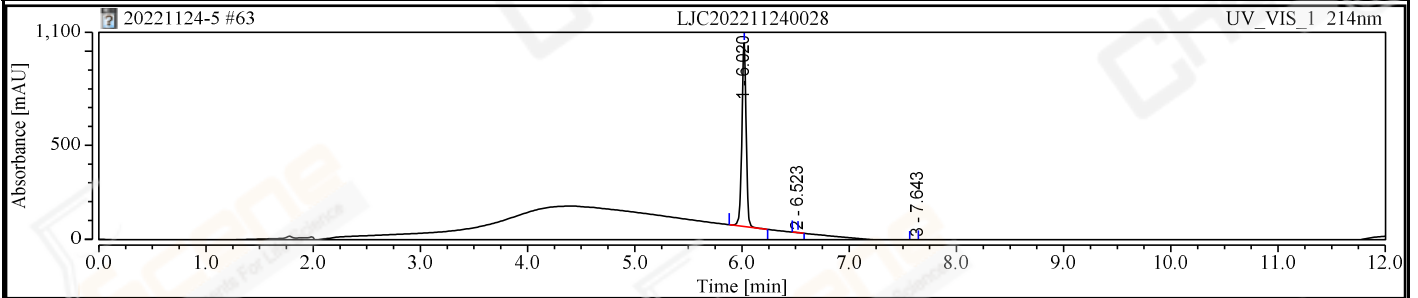

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	6.020	44.452	976.599	116871	6.75	0.94	99.471	
2	6.523	0.019	0.390	110028	14.63	1.04	0.042	
3	7.643	0.218	4.657	168746	n.a.	1.00	0.488	
Total:		44.689	981.645		21.38			