
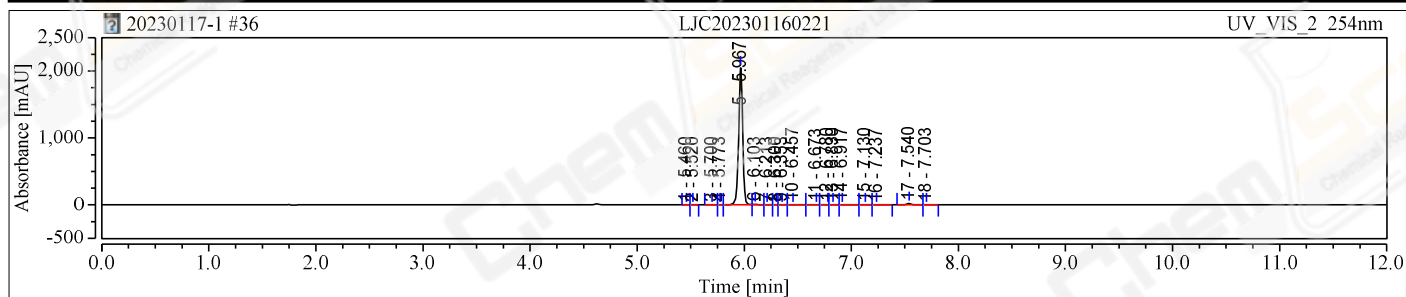


Chromatogram and Results

Sample ID:	LJC202301160221	CAS NO.:	14544-47-9
Batch No:		Channel:	UV_VIS_1
Vial Number:	BE2	Wavelength:	214.0
Injection Type:	Unknown	Injection Volume:	5.00
Instrument:	LC10411	Injection Time:	17/01/2023 16:51
Instrument Method:	10-80A-12min	InstMeth.creation_t	15/06/2022 08:55
Processing Method:	LJC202301160221	Last update_time:	18/01/2023 10:31
seq.creation_operator	Msunwj		
chrom://ahqc016/CMDATA/Instrument Data/LC10411/Leyan/Sequence/20230117-1.seq/891.smp/UV_VIS_1.channel/UV_VIS_1.chm			

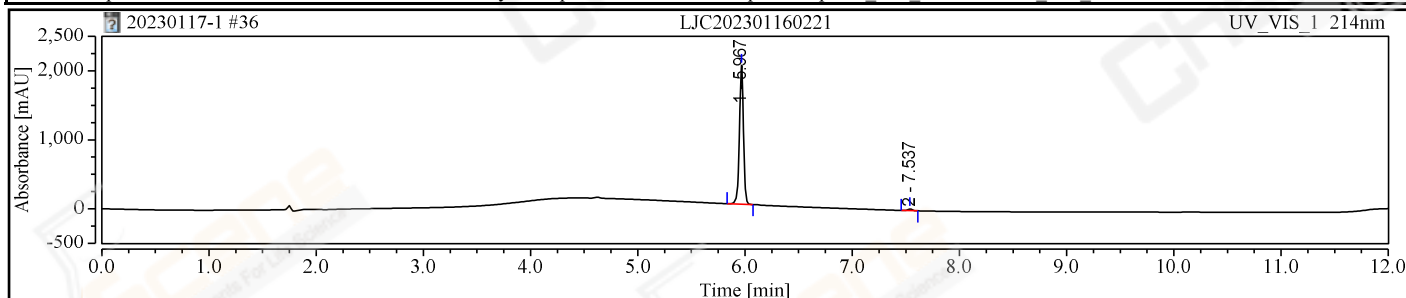

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	5.967	89.195	2013.770	121022	22.18	0.95	98.721	
2	7.537	1.156	24.886	170778	n.a.	1.03	1.279	
Total:		90.351	2038.656		22.18			

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	5.460	0.046	1.099	96330	0.81	n.a.	0.050	
2	5.520	0.031	0.734	79916	2.47	n.a.	0.034	
3	5.700	0.052	1.171	113946	0.53	n.a.	0.056	
4	5.773	0.010	0.230	12186	1.40	n.a.	0.011	
5	5.967	89.980	2046.966	123572	1.71	0.95	97.880	
6	6.103	0.366	6.418	70156	0.36	n.a.	0.398	
7	6.213	0.065	0.967	2316	0.10	n.a.	0.071	
8	6.300	0.031	0.609	430	0.08	n.a.	0.033	
9	6.353	0.058	0.968	56635	1.07	n.a.	0.063	
10	6.457	0.119	1.850	89325	0.94	n.a.	0.129	
11	6.673	0.031	0.307	5077	0.28	n.a.	0.034	
12	6.780	0.033	0.533	5231	0.21	n.a.	0.036	
13	6.830	0.061	0.981	66071	0.61	n.a.	0.067	
14	6.917	0.041	0.380	24789	1.63	n.a.	0.045	
15	7.130	0.032	0.542	108551	1.05	n.a.	0.035	
16	7.237	0.017	0.225	60671	3.17	n.a.	0.019	
17	7.540	0.942	19.396	166032	0.78	0.97	1.025	
18	7.703	0.013	0.168	7915	n.a.	n.a.	0.014	
Total:		91.929	2083.543		17.19			