
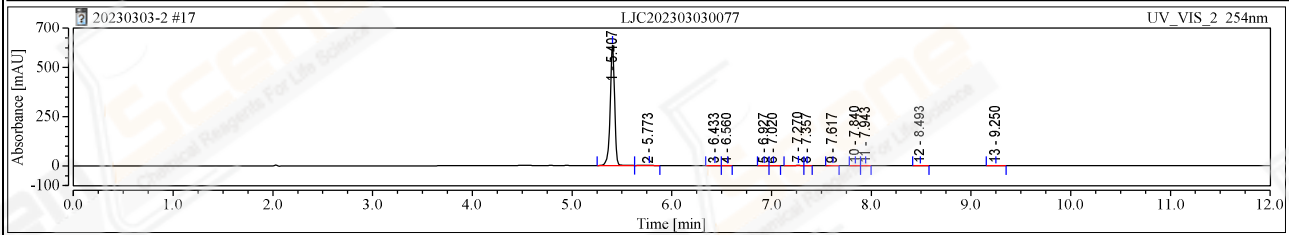


## Chromatogram and Results

Sample ID:	LJC202303030077	CAS NO.:	10132-07-7
Batch No:		Channel:	UV_VIS_1
Vial Number:	BB8	Wavelength:	214.0
Injection Type:	Unknown	Injection Volume:	2.00
Instrument:	LC10410	Injection Time:	03/03/2023 20:38
Instrument Method:	10-80A-12min(LP-HPLC)	InstMeth.creation:	115/04/2022 17:33
Processing Method:	LJC202303030077	Last update_time:	06/03/2023 11:19
seq.creation_operator:	Azhangl		

an/Sequence/202303/20230303-2.seq/143.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

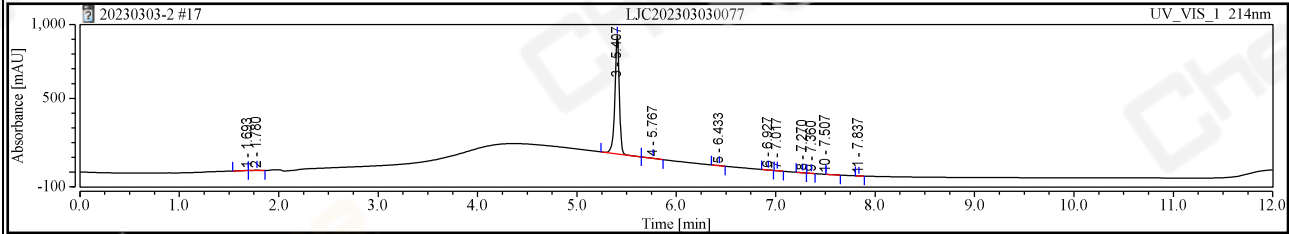

No.	Retention Time [min]	Area [mAU*min]	Height [mAU]	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	1.693	0.026	0.000	10906	1.15	n.a.	0.062	
2	1.780	0.192	3.245	6822	43.84	0.92	0.456	
3	5.407	41.585	802.347	74462	3.12	0.87	98.867	
4	5.767	0.108	1.080	23079	5.97	0.91	0.257	
5	6.433	0.052	1.141	130006	6.71	0.87	0.124	
6	6.927	0.011	0.225	134258	1.34	0.90	0.026	
7	7.017	0.005	0.138	231012	3.99	1.36	0.012	
8	7.270	0.010	0.230	180462	1.33	0.83	0.024	
9	7.360	0.006	0.153	195406	2.07	0.91	0.015	
10	7.507	0.061	0.000	159058	4.81	n.a.	0.145	
11	7.837	0.005	0.124	256125	n.a.	1.10	0.011	
<b>Total:</b>		<b>42.061</b>	<b>808.682</b>		<b>74.33</b>			

No.	Retention Time [min]	Area [mAU*min]	Height [mAU]	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	5.407	30.635	610.665	79626	3.04	0.87	99.252	
2	5.773	0.085	0.782	19597	5.51	0.84	0.274	
3	6.433	0.022	0.447	118481	1.75	0.85	0.070	
4	6.560	0.004	0.082	140148	4.76	0.88	0.012	
5	6.927	0.008	0.155	109190	1.24	0.88	0.026	
6	7.020	0.015	0.353	178379	3.60	1.05	0.047	
7	7.270	0.052	1.089	160610	1.29	0.81	0.170	
8	7.357	0.003	0.086	230179	3.17	1.16	0.011	
9	7.617	0.017	0.260	88421	2.42	0.86	0.056	
10	7.840	0.004	0.090	146788	1.37	0.96	0.014	
11	7.943	0.004	0.098	210878	7.08	1.06	0.014	
12	8.493	0.004	0.066	155324	7.13	1.00	0.013	
13	9.250	0.012	0.147	86233	n.a.	1.03	0.040	
<b>Total:</b>		<b>30.866</b>	<b>614.319</b>		<b>42.36</b>			