
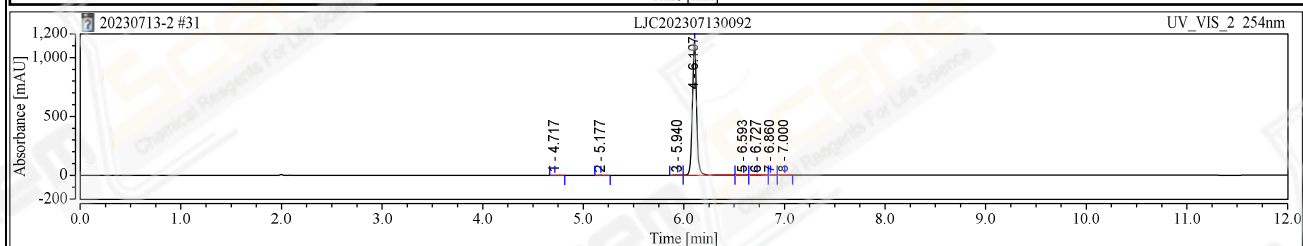


Chromatogram and Results

Sample ID: LJC202307130092	Comment: 20230713278943-1103839AH-LC111
CAS NO.: 1532517-95-5	Channel: UV_VIS_1
Vial Number: RB6	Wavelength: 214.0
Injection Type: Unknown	Injection Volume: 5.00
Instrument: LC10410	Injection Time: 13/07/2023 19:05
Instrument Method: 10-80A-12min(LP-HPLC)	InstMeth.creation: 15/04/2022 17:33
Processing Method: LJC202307130092	Last update_time: 14/07/2023 10:41
seq.creation_operator: Azhangl	
/Sequence/202307/20230713-2.seq/220.smp/UV_VIS_1.channel/UV_VIS_1.chm	

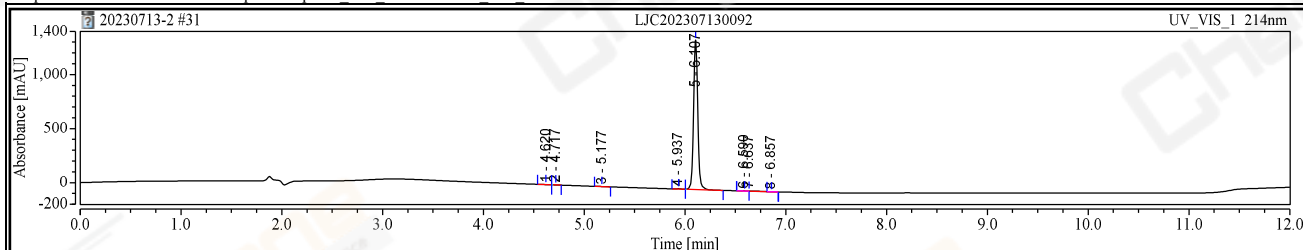

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	4.620	0.028	0.346	20088	0.87	n.a.	0.042	
2	4.717	0.023	0.429	43044	5.50	n.a.	0.034	
3	5.177	0.034	0.685	73383	10.11	1.18	0.051	
4	5.937	0.168	3.522	103108	2.32	n.a.	0.254	
5	6.107	65.745	1382.506	113746	6.65	1.02	99.363	
6	6.590	0.018	0.317	n.a.	n.a.	n.a.	0.027	
7	6.637	0.141	0.062	93233	n.a.	1.72	0.214	
8	6.857	0.010	0.182	n.a.	n.a.	n.a.	0.014	
Total:		66.167	1388.050		25.45			

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	4.717	0.006	0.142	86259	6.58	1.04	0.011	
2	5.177	0.016	0.322	74925	10.12	1.20	0.029	
3	5.940	0.118	2.457	99986	2.26	n.a.	0.217	
4	6.107	54.227	1137.354	113332	4.87	1.02	99.472	
5	6.593	0.023	0.305	42893	1.17	n.a.	0.043	
6	6.727	0.100	1.371	72375	0.50	n.a.	0.184	
7	6.860	0.009	0.142	4069	0.54	n.a.	0.017	
8	7.000	0.015	0.231	92626	n.a.	n.a.	0.027	
Total:		54.515	1142.324		26.04			