
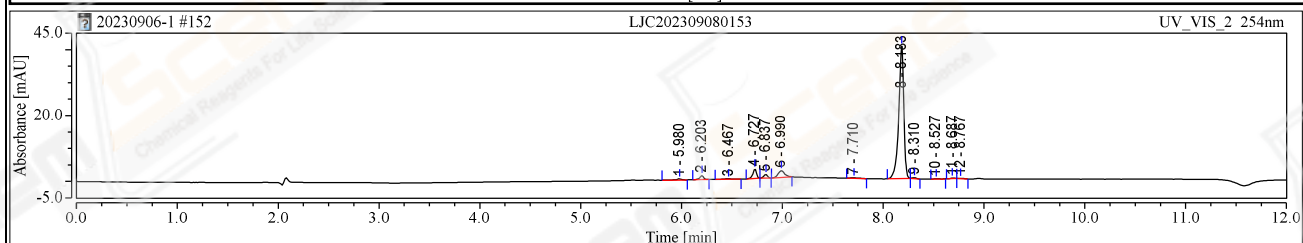


Chromatogram and Results

Sample ID: LJC202309080153	Comment: 1064191-20230908302818AH-LC111
CAS NO.: 488-23-3	Channel: UV_VIS_1
Vial Number: GC3	Wavelength: 214.0
Injection Type: Unknown	Injection Volume: 1.00
Instrument: LC10410	Injection Time: 08/09/2023 21:07
Instrument Method: 10-80A-12min(LP-HPLC)	InstMeth.creation: 15/04/2022 17:33
Processing Method: LJC202309070175	Last update_time: 11/09/2023 09:00
seq.creation_operator: Azhangl	

ence/202309/Sequence/20230906-1.seq/956.smp/UV_VIS_1.channel/UV_VIS_1.chm

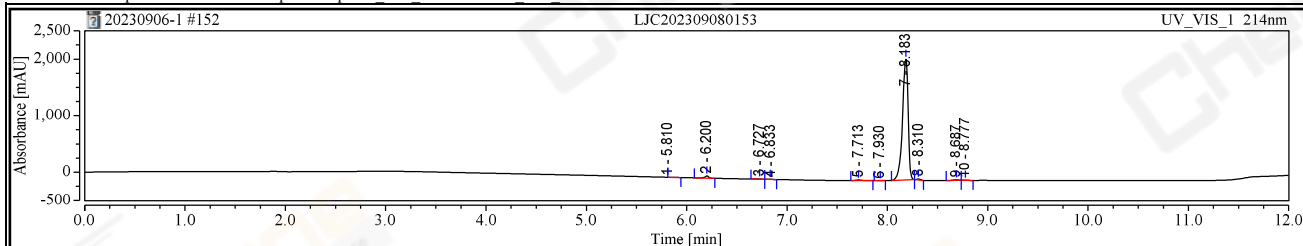

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	5.810	0.117	0.000	36622	4.20	n.a.	0.082	
2	6.200	1.755	40.801	148725	8.09	0.85	1.227	
3	6.727	0.270	6.321	166888	1.59	0.84	0.189	
4	6.833	0.115	2.620	160481	11.69	1.01	0.080	
5	7.713	0.553	9.294	140525	2.83	1.24	0.386	
6	7.930	0.017	0.383	201719	3.07	0.98	0.012	
7	8.183	138.678	2138.312	119653	1.54	0.80	96.932	
8	8.310	0.760	17.879	228538	4.91	1.08	0.531	
9	8.687	0.586	11.035	171622	1.01	0.82	0.410	
10	8.777	0.217	3.766	138564	n.a.	1.38	0.152	
Total:		143.068	2230.411		38.94			

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	5.980	0.021	0.355	126570	3.39	0.68	0.755	
2	6.203	0.056	1.300	148061	2.68	0.81	2.005	
3	6.467	0.017	0.169	38590	2.64	1.00	0.617	
4	6.727	0.124	2.920	168102	1.67	0.85	4.451	
5	6.837	0.048	1.149	171412	1.69	0.89	1.715	
6	6.990	0.155	2.061	58905	5.57	1.12	5.567	
7	7.710	0.015	0.163	46378	4.13	1.36	0.528	
8	8.183	2.321	40.305	144005	1.63	0.81	83.118	
9	8.310	0.013	0.299	229716	2.67	1.12	0.458	
10	8.527	0.005	0.070	133788	1.86	1.43	0.164	
11	8.687	0.010	0.213	195694	0.95	0.88	0.366	
12	8.767	0.007	0.128	149343	n.a.	1.45	0.255	
Total:		2.792	49.132		28.87			